

## **BLANK PAGE**



## भारतीय मानक

द्रवचालित तरल पावर — द्रव — ठोस कणों से संदूषण के स्तर को कूटबद्ध करने की पद्धति (पहला पुनरीक्षण)

### Indian Standard

# HYDRAULIC FLUID POWER — FLUIDS — METHOD FOR CODING THE LEVEL OF CONTAMINATION BY SOLID PARTICLES

(First Revision)

ICS 23.100.60; 75.120

© BIS 2013

BUREAU OF INDIAN STANDARDS MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG NEW DELHI 110002

January 2013 Price Group 4

#### NATIONAL FOREWORD

This Indian Standard (First Revision) which is identical with ISO 4406: 1999 'Hydraulic fluid power — Fluids — Method for coding the level of contamination by solid particles' issued by the International Organization for Standardization (ISO) was adopted by the Bureau of Indian Standards on the recommendation of the Fluid Power Systems Sectional Committee and approval of the Production and General Engineering Division Council.

This standard was originally published as IS 13542: 1992 'Hydraulic fluid power — Contamination analysis — Method of reporting analysis data' based on ISO 3938: 1986 'Hydraulic fluid power — Contamination analysis — Method of reporting analysis data' and ISO 4406: 1987 'Hydraulic fluid power — Fluids — Method for coding the level of contamination by solid particles'. The first revision has been harmonized with ISO 4406: 1999 by adoption under dual numbering system to make pace with the latest developments that have taken place at international level.

The text of ISO Standard has been approved as suitable for publication as an Indian Standard without deviations. Certain terminology and conventions are, however, not identical to those used in Indian Standards. Attention is particularly drawn to the following:

- a) Wherever the words 'International Standard' appear referring to this standard, they should be read as 'Indian Standard'.
- b) Comma (,) has been used as a decimal marker while in Indian Standards the current practice is to use a point (.) as the decimal marker.

The technical committee has reviewed the provisions of the following International Standards referred in this adopted standard and has decided that they are acceptable for use in conjunction with this standard:

International Standard	Title
ISO 4407 : 1991 <sup>1)</sup>	Hydraulic fluid power — Fluid contamination — Determination of particulate contamination by the counting method using a microscope
ISO 11171 : 1999 <sup>2)</sup>	eq:Hydraulic fluid power — Calibration of automatic particle counters for liquids
ISO 11500 : 1997 <sup>3)</sup>	Hydraulic fluid power — Determination of the particulate contamination by automatic counting using the light-extinction principle

Annex A forms a normative part of this standard.

For the purpose of deciding whether a particular requirement of this standard is complied with, the final value, observed or calculated, expressing the result of a test or analysis, shall be rounded off in accordance with IS 2: 1960 'Rules for rounding off numerical values (*revised*)'. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

<sup>&</sup>lt;sup>1)</sup> Since revised in 2002.

<sup>&</sup>lt;sup>2)</sup> Since revised in 2010.

<sup>&</sup>lt;sup>3)</sup> Since revised in 2008.

## Indian Standard

# HYDRAULIC FLUID POWER — FLUIDS — METHOD FOR CODING THE LEVEL OF CONTAMINATION BY SOLID PARTICLES

(First Revision)

#### 1 Scope

This International Standard specifies the code to be used in defining the quantity of solid particles in the fluid used in a given hydraulic fluid power system.

#### 2 Normative references

The following normative documents contain provisions which, through reference in this text, constitute provisions of this International Standard. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. However, parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the normative documents indicated below. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.

ISO 4407:1991, Hydraulic fluid power — Fluid contamination — Determination of particulate contamination by the counting method using a microscope.

ISO 11171:1999, Hydraulic fluid power — Calibration of automatic particle counters for liquids.

ISO 11500:1997, Hydraulic fluid power — Determination of particulate contamination by automatic counting using the light extinction principle.

#### 3 Code definition

#### 3.1 General

The purpose of this code is to simplify the reporting of particle count data by converting the numbers of particles into broad classes or codes, where an increase in one code is generally a doubling of the contamination level.

The original code in accordance with ISO 4406:1987 stated the reporting at two sizes,  $\geqslant 5~\mu m$  and  $\geqslant 15~\mu m$ , but the sizes in this revision have been changed to account for the use of a different calibration standard for optical automatic particle counters. The reported sizes are  $\geqslant 4~\mu m(c)$ ,  $\geqslant 6~\mu m(c)$  and  $\geqslant 14~\mu m(c)$ , the last two of these being equivalent to the  $5~\mu m$  and  $15~\mu m$  particle sizes obtained using the ISO 4402:1991 method of calibrating automatic particle counters. ISO 4402:1991 has been replaced by ISO 11171:1999. Throughout this International Standard, the use of  $\mu m(c)$  means that particle size measurements are carried out using an automatic particle counter which has been calibrated in accordance with ISO 11171.

Measurement of particles using an optical microscope as specified in ISO 4407:1991 establishes the size of a particle as being equal to its longest dimension, whereas an automatic particle counter derives the size of an equivalent particle from its cross-sectional area, a value different in most cases from that determined using a microscope. The particle sizes to be reported for measurement by microscope,  $\geqslant 5 \, \mu m$  and  $\geqslant 15 \, \mu m$ , are unchanged from those specified in ISO 4406:1987.

CAUTION — Particle counts are affected by a variety of factors. These factors include procurement of sample, particle counting accuracy, and the sample container, where used, and its cleanliness. Proper care should be taken during sample procurement to ensure that the sample obtained is representative of the fluid circulation in the system.

#### 3.2 Basis of code

The code for contamination levels using automatic particle counters comprises three scale numbers, which permit the differentiation of the dimension and the distribution of the particles as follows:

- the first scale number represents the number of particles equal to or larger than 4 μm(c) per millilitre of fluid;
- the second scale number represents the number of particles equal to or larger than 6 μm(c) per millilitre of fluid;
- the third scale number represents the number of particles equal to or larger than 14 μm(c) per millilitre of fluid.

The code for microscope counting comprises two scale numbers using 5 μm and 15 μm.

#### 3.3 Allocation of scale numbers

- **3.3.1** The scale numbers are allocated according to the number of particles counted per millilitre of the fluid sample (see Table 1).
- **3.3.2** A step ratio of generally two, as given between the upper and lower limits for the number of particles per millilitre in Table 1, has been adopted to keep the number of scale numbers within a reasonable limit and to ensure that each step is meaningful.

#### 3.4 Determination of code using automatic particle counter analysis

- **3.4.1** Counting shall be undertaken in accordance with ISO 11500 or another recognised method, using an automatic particle counter calibrated to ISO 11171.
- 3.4.2 A scale number shall be allocated to the number of particles equal to or larger than 4 μm(c).
- 3.4.3 A second scale number shall be allocated to the number of particles equal to or larger than 6 μm(c).
- **3.4.4** A third scale number shall be allocated to the number of particles equal to or larger than 14 μm(c).
- **3.4.5** The three numbers shall be written one after the other and separated by oblique strokes (slashes).
- EXAMPLE A code of 22/18/13 signifies that there are more than 20 000 and up to and including 40 000 particles equal to or larger than 4  $\mu$ m(c), more than 1 300 and up to and including 2 500 particles equal to or larger than 6  $\mu$ m(c) and more than 40 and up to and including 80 particles equal to or larger than 14  $\mu$ m(c) in 1 ml of a given fluid sample.
- **3.4.6** When applicable, include either a "\*" (too numerous to count) or a "—" (no requirement to count) notation when reporting the scale number.
- EXAMPLE 1 \*/19/14 means that this sample has too many particles equal to or larger than 4  $\mu$ m(c) to count.
- EXAMPLE 2 —/19/14 means that there was no requirement to count particles equal to or larger than 4  $\mu$ m(c).

Table 1 — Allocation of scale numbers

Number of part	icles per millilitre	Scale number
More than	Up to and including	
2 500 000		>28
1 300 000	2500000	28
640 000	1 300 000	27
320 000	640 000	26
160 000	320 000	25
80 000	160 000	24
40 000	80 000	23
20 000	40 000	22
10 000	20 000	21
5 000	10 000	20
2500	5 0 0 0	19
1 300	2500	18
640	1 300	17
320	640	16
160	320	15
80	160	14
40	80	13
20	40	12
10	20	11
5	10	10
2,5	5	9
1,3	2,5	8
0,64	1,3	7
0,32	0,64	6
0,16	0,32	5
0,08	0,16	4
0,04	0,08	3
0,02	0,04	2
0,01	0,02	1
0,00	0,01	0

NOTE Reproducibility below scale number 8 is affected by the actual number of particles counted in the fluid sample. Raw counts should be more than 20 particles. If this is not possible, then refer to 3.4.7.

**3.4.7** When the raw data in one of the size ranges results in a particle count of fewer than 20 particles, the scale number for that size range shall be labelled with the symbol  $\geq$ .

EXAMPLE A code of  $14/12/\geqslant 7$  signifies that there are more than 80 and up to and including 160 particles equal to or larger than 4 µm(c) per millilitre and more than 20 and up to and including 40 particles equal to or larger than 6 µm(c) per millilitre. The third part of the code,  $\geqslant 7$ , indicates that there are more than 0,64 and up to and including 1,3 particles equal to or larger than 14 µm(c) per millilitre, but less than 20 particles were counted, which lowers statistical confidence. Because of this lower confidence, the 14 µm(c) part of the code could actually be higher than 7, indicating a particle count more than 1,3 particles per millilitre.

#### 3.5 Determination of code using microscope sizing

- **3.5.1** Counting shall be undertaken in accordance with ISO 4407.
- **3.5.2** A scale number shall be allocated to the number of particles equal to or larger than 5 μm.
- **3.5.3** A second scale number shall be allocated to the number of particles equal to or larger than 15 μm.
- **3.5.4** In order to relate to counts obtained with an automatic particle counter, the code shall be stated in three-part form with the first part given as a "—", e.g. -/18/13.

#### 4 Identification statement (reference to this International Standard)

Use the following statement in test reports, catalogues and sales literature when electing to comply with this International Standard:


"Solid contaminant code conforms to ISO 4406:1999, *Hydraulic fluid power — Fluids — Method for coding the level of contamination by solid particles.*"

## Annex A (normative)

### Graphical presentation of the code number

For automatic particle counter analysis, the contaminant code is determined by allocating a first scale number to the total number of particles equal to or larger than 4  $\mu$ m(c), allocating a second scale number to the total number of particles equal to or larger than 6  $\mu$ m(c) and allocating a third scale number to the total number of particles equal to or larger than 14  $\mu$ m(c), and then writing these three numbers one after another separated by oblique strokes (slashes). For an example, see 22/18/13 in Figure A.1. For analysis by microscope, use a "—" in place of the first scale number and allocate the second and third numbers based on the counts at 5  $\mu$ m and 15  $\mu$ m, respectively.

Interpolation is acceptable, extrapolation is not permissible.

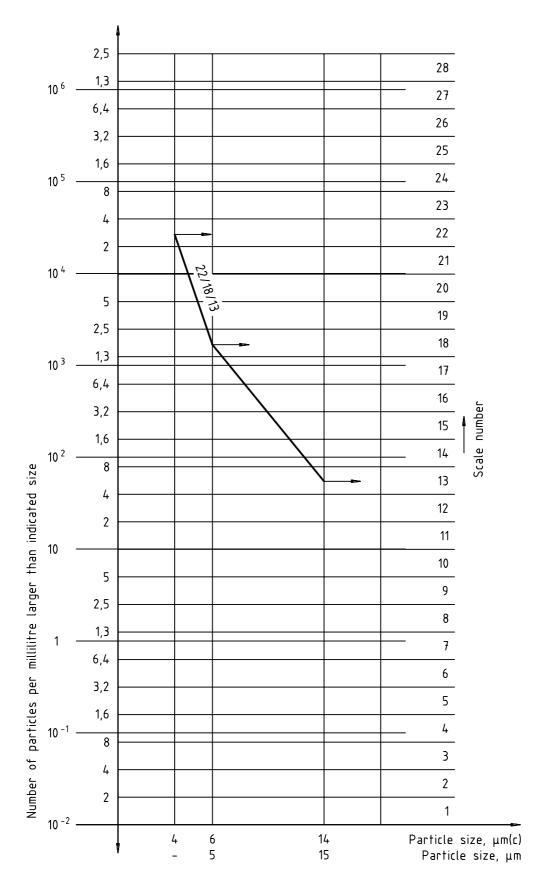

NOTE Quote scale number at 4  $\mu$ m(c), 6  $\mu$ m(c) and 14  $\mu$ m(c) levels for automatic particle counters, and at 5  $\mu$ m and 15  $\mu$ m for microscope counting.

Figure A.1

## **Bibliography**

[1] ISO 4021:1992, Hydraulic fluid power — Particulate contamination analysis — Extraction of fluid samples from lines of an operating system.

#### **Bureau of Indian Standards**

BIS is a statutory institution established under the *Bureau of Indian Standards Act*, 1986 to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

#### Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

#### **Review of Indian Standards**

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard along with amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the latest issue of 'BIS Catalogue' and 'Standards: Monthly Additions'.

This Indian Standard has been developed from Doc No.: PGD 16 (1179).

#### **Amendments Issued Since Publication**

Amendment No.	Date of Issue Text Affected	

#### **BUREAU OF INDIAN STANDARDS**

#### **Headquarters:**

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110002

Telephones: 2323 0131, 2323 3375, 2323 9402 Website: www.bis.org.in

Regional Offices:	Telephones
Central: Manak Bhavan, 9 Bahadur Shah Zafar Marg NEW DELHI 110002	( 2323 7617 ( 2323 3841
Eastern: 1/14, C.I.T. Scheme VII M, V.I.P. Road, Kankurgachi KOLKATA 700054	2337 8499, 2337 8561 2337 8626, 2337 9120
Northern: SCO 335-336, Sector 34-A, CHANDIGARH 160022	(260 3843 (260 9285
Southern: C.I.T. Campus, IV Cross Road, CHENNAI 600113	( 2254 1216, 2254 1442 2254 2519, 2254 2315
Western: Manakalaya, E9 MIDC, Marol, Andheri (East) MUMBAI 400093	(2832 9295, 2832 7858 (2832 7891, 2832 7892

**Branches:** AHMEDABAD. BANGALORE. BHOPAL. BHUBANESHWAR. COIMBATORE. DEHRADUN. FARIDABAD. GHAZIABAD. GUWAHATI. HYDERABAD. JAIPUR. KANPUR. LUCKNOW. NAGPUR. PARWANOO. PATNA. PUNE. RAJKOT. THIRUVANATHAPURAM. VISAKHAPATNAM.