

इंटरनेट

मानक

Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 5584 (1970): Syringe, Hypodermic, Cartridge, Dental, Pivot Breech Cap Type [MHD 8: Dentistry]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”


BLANK PAGE





Indian Standard
**SPECIFICATION FOR SYRINGE, HYPODERMIC,
 CARTRIDGE, DENTAL, PIVOT BREECH CAP TYPE**

1. **Scope** — Dimensions and other requirements for dental hypodermic cartridge syringe of pivot breech cap type to be used with cartridge needles conforming to IS: 5180-1969*.
2. **Shape and Dimensions** — As shown in Fig. 1 and 2.

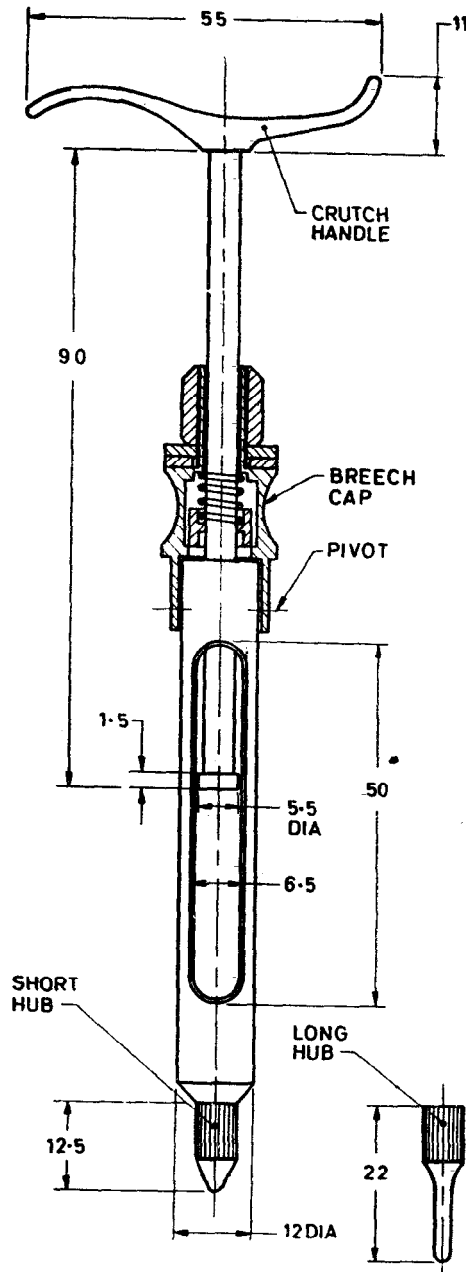

All dimensions in millimetres.

FIG. 1 SYRINGE, HYPODERMIC, CARTRIDGE, PIVOT BREECH CAP TYPE


*Specification for needles, hypodermic, dental.

Adopted 2 April 1970

© November 1970

Price: RS 5.00

Gr 1

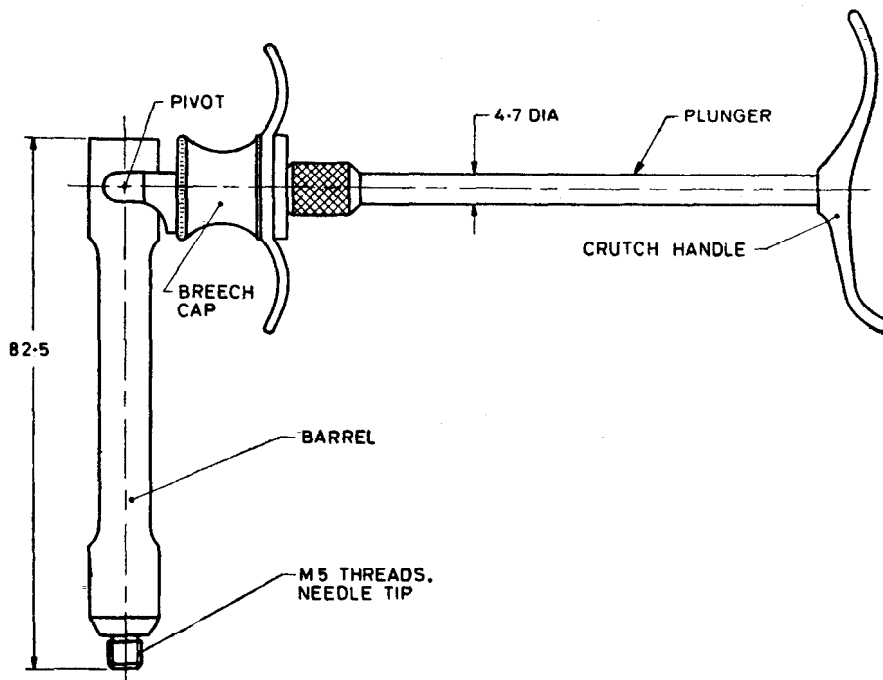

All dimensions in millimetres.

FIG. 2 SYRINGE, HYPODERMIC, CARTRIDGE, SHOWING BREECH ACTION

3. Material

3.1 Barrel — Brass tube conforming to Alloy No. 2 (Designation CuZn39) of IS : 407-1966*. The outside diameter and wall thickness of the brass tube shall be 12 and 0.8 mm respectively.

3.2 All other Components — Brass rods conforming to Designation CuZn38Pb3 of IS : 319-1968†.

4. Requirements

4.1 Breech Cap — Syringes shall be breech loading type and the breech cap shall pivot to allow the cartridge, 77 mm long and 9.1 mm in diameter containing anaesthetic solution to be freely inserted into the barrel of the syringe and shall contain a swivel type finger hold grip.

4.2 Needle Tip of the Barrel — Shall have M5 threads and counterbored to form a seat for the head on the needle.

4.3 Hubs — One short and one long hub shall be provided with each syringe. The hub shall be bored for cartridge needles specified in IS : 5180-1969‡, counterbored for the seat for the head on the needle, and shall have M5 threads, to fit the needle tip of the barrel.

5. Workmanship and Finish

5.1 The finished syringe shall be free from defects which impair their appearance, use or durability.

5.2 The heads of the pivots shall be flush with the breech cap and shall be of such construction that they will not become dislodged when in use. Screws if used as pivot, shall be expanded or swelled so that they cannot be removed with a screw driver.

5.3 The syringe shall be easily and readily disassembled for complete sterilization.

5.4 The plunger shall be securely brazed to handle and finished smooth.

5.5 The syringe shall be plated chromium over nickel and the plating shall conform to Service Grade No. 2 of IS : 4827-1968§.

6. Marking — Each syringe shall be marked with manufacturer's name, initials or trade-mark; and country of manufacture.

6.1 ISI Certification Marking — Details available from the Indian Standards Institution ,

7. Packing — The syringe shall be either wrapped in wax paper or put in polyethylene bag and then packed in cartons in accordance with trade practice or the packing may be done as agreed to between the purchaser and the supplier.

*Specification for brass tubes for general purposes (second revision).

†Specification for free-cutting brass rods and sections (second revision).

‡Specification for needles, hypodermic, dental.

§Specification for electroplated coatings of nickel and chromium on copper and copper alloys.