

इंटरनेट

मानक

### Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 6901 (2009): Gas welding equipment - Pressure regulators for gas cylinders used in welding, cutting and allied processes up to 300 bar [MTD 11: Welding General]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”



BLANK PAGE



*भारतीय मानक*

गैस वेल्डिंग उपस्कर — वेल्डिंग, कटिंग और संबद्ध प्रक्रियाओं के लिए प्रयुक्त 300 बार तक के गैस सिलिंडरों के लिए दाब रेगुलेटर  
( दूसरा पुनरीक्षण )

*Indian Standard*

GAS WELDING EQUIPMENT — PRESSURE  
REGULATORS FOR GAS CYLINDERS USED IN  
WELDING, CUTTING AND ALLIED PROCESSES  
UP TO 300 BAR  
( *Second Revision* )

ICS 77 160

© BIS 2009

**BUREAU OF INDIAN STANDARDS**  
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG  
NEW DELHI 110002

## NATIONAL FOREWORD

This Indian Standard (Second Revision) which is identical with ISO 2503 : 1998 'Gas welding equipment — Pressure regulators for gas cylinders used in welding, cutting and allied processes up to 300 bar' issued by the International Organization for Standardization (ISO) was adopted by the Bureau of Indian Standards on the recommendation of the Welding General Sectional Committee and approval of the Metallurgical Engineering Division Council.

This standard was originally published in 1973 and subsequently revised in 1981. This revision of the standard has been taken up to align it with ISO 2503 : 1998 by adoption, under dual numbering system.

This standard covers all the important aspects of pressure regulators for gas cylinders including the safety aspects. Certain aspects of physical characteristics that is pressure, flow rate and equipment classes for different types of industrial gases used are specified very clearly.

The text of ISO Standard has been approved as suitable for publication as an Indian Standard without deviations. Certain conventions are, however, not identical to those used in Indian Standards. Attention is particularly drawn to the following:

- a) Wherever the words 'International Standard' appear referring to this standard, they should be read as 'Indian Standard'.
- b) Comma (,) has been used as a decimal marker, while in Indian Standards, the current practice is to use a point (.) as the decimal marker.

BIS Certification Marking clause is given in National Annex A.

In this adopted standard, reference appears to certain International Standards for which Indian Standards also exist. The corresponding Indian Standards which are to be substituted in their places are listed below along with their degree of equivalence for the editions indicated:

<i>International Standard</i>	<i>Corresponding Indian Standard</i>	<i>Degree of Equivalence</i>
ISO 554 : 1976 Standard atmospheres for conditioning and/or testing — Specifications	IS 196 : 1966 Atmospheric conditions for testing ( <i>revised</i> )	Technically Equivalent
ISO 3253 : 1998 Gas welding equipment — Hose connections for equipment for welding cutting and allied processes	IS 6016 : 2008 Gas welding equipment — Hose connections for equipment for welding, cutting and allied processes ( <i>second revision</i> )	Identical
ISO 5171 : 1995 Pressure gauges used in welding, cutting and allied processes	IS 3624 : 1987 Specification for pressure and vacuum gauges ( <i>second revision</i> )	Technically Equivalent

The technical committee responsible for the preparation of this standard has reviewed the provisions of the following International Standards and has decided that they are acceptable for use in conjunction with this standard.

(Continued on third cover)

*Indian Standard*

**GAS WELDING EQUIPMENT — PRESSURE  
REGULATORS FOR GAS CYLINDERS USED IN  
WELDING, CUTTING AND ALLIED PROCESSES  
UP TO 300 BAR**

*( Second Revision )*

## 1 Scope

This International Standard specifies requirements for single or two-stage pressure regulators for connections to gas cylinders normally used for compressed gases up to 300 bar<sup>1)</sup> (30 MPa), for dissolved acetylene, for liquefied petroleum gases (LPG), methylacetylene-propadiene-mixtures (MPS) and carbon dioxide (CO<sub>2</sub>) used in welding, cutting and allied processes.

## 2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All Standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 554 1976, *Standard atmospheres for conditioning and/or testing — Specifications*

ISO 3253 1998, *Gas welding equipment — Hose connections for equipment for welding, cutting and related processes*

ISO 5171 1995, *Pressure gauges used in welding, cutting and allied processes*

ISO/TR 7470 1988, *Valve outlets for gas cylinders — List of provisions which are either standardized or in use*

ISO 9090 1989, *Gas tightness of equipment for gas welding and allied processes*

ISO 9539 1988, *Materials for equipment used in gas welding, cutting and allied processes*

## 3 Definition

For the purposes of this International Standard, the following definition applies


**3.1 pressure regulator:** Device for regulating a generally variable inlet pressure to an as constant as possible outlet pressure.

---

1) 300 bar relates to maximum cylinder charging pressure at 15 °C

#### 4 Terminology

The terms relating to pressure regulators are given in the key to figure 1 given in table 1. The diagram of the pressure regulator is an example only.

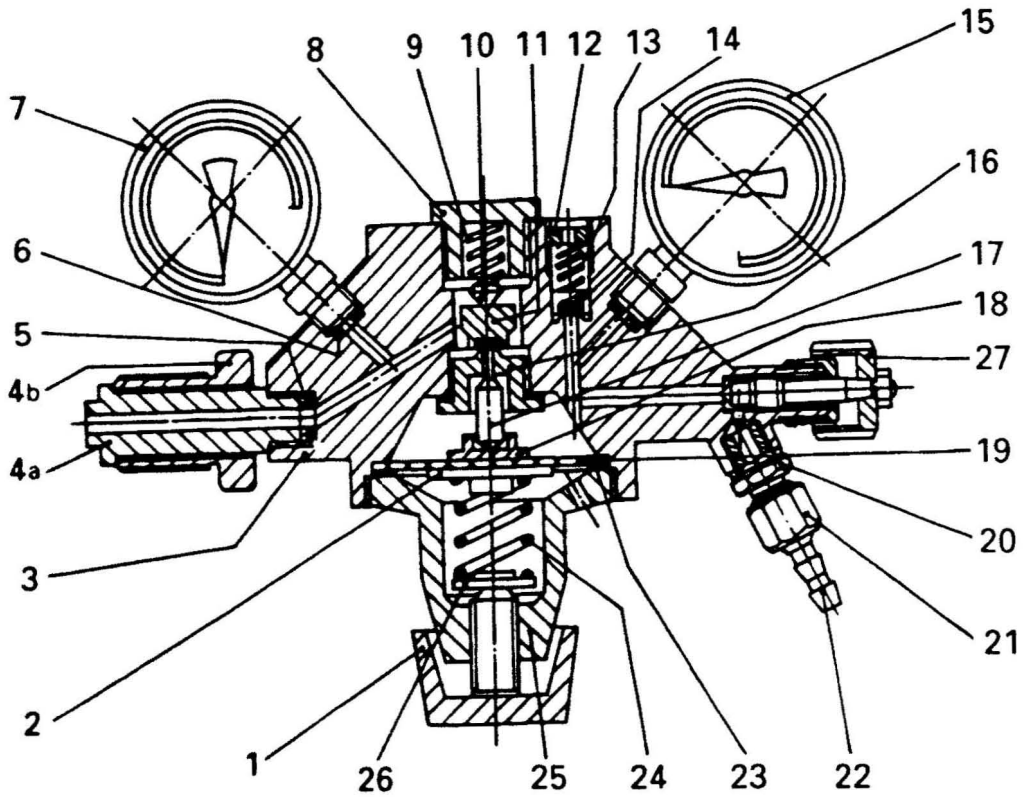

#### NOTES

- 1 Parts 12, 13 and 14 are components of the relief valve
- 2 Part 27 is an outlet valve and its installation is optional, see 6.2.4.
- 3 Parts 4a and 4b of the drawing are examples and are not specified. Other types of inlet connection pieces are also in use.

**Figure 1 — Diagram of a pressure regulator and designation of its components**

Table 1 — List of terms

No.	English	French	German
1	pressure adjusting screw	vis de réglage	Einstellschraube
2	spring plate	plateau de membrane	Federteller
3	body	corps	Körper
4a	inlet stem	raccord d'entrée	Eingangsstutzen
4b	inlet nut	écrou flottant raccord d'entrée	Schraubverbindung
5	inlet filter	filtre d'entrée	Eintrittsfilter
6	seating washer	joint de manometre	Manometeranschluß- Dichtungsring
7	high-pressure gauge	manometre haute pression (amont)	Hochdruckmanometer
8	pressure regulator valve cap	bouchon de clapet	Regelventilkappe
9	pressure regulator valve spring	ressort de clapet	Regelventilfeder
10	spring centre	appui mobile de centrage du ressort de clapet	Regelventil-Federteller
11	pressure regulator valve	clapet	Regelventil
12	relief valve cap	vis de réglage de la soupape de securite	Einstellschraube des Abblaseventils
13	relief valve spring	ressort de soupape de securite	Feder für Abblaseventil
14	relief valve seat	clapet de soupape de securite	Abblaseventilsitz
15	low-pressure gauge	manometre basse pression (aval)	Niederdruckmanometer
16	pressure regulator valve seat	siège	Regelventilsitz
17	pressure regulator valve pin	poussoir	Regelventilstift
18	diaphragm plate	plateau d'appui du poussoir	Membranteller
19	diaphragm	membrane	Membran
20	outlet connection piece	raccord de sortie (mamelon fileté)	Abgangsstutzen
21	union nut	écrou de douille	Überwurfmutter
22	hose tail	douille porte-tuyau	Schlauchtüle
23	diaphragm seal	joint de membrane	Membrangleitung
24	pressure regulator spring	ressort de détente	Stellfeder
25	pressure regulator cover	couvercle	Federdeckel
26	pressure regulator spring plate	appui mobile de centrage du ressort de détente	Stellfederteller
27	outlet valve	robinet de sortie	Absperrventil



## 5 Units

### 5.1 Pressure

The pressures measured are gauge pressures<sup>2)</sup> and are expressed in bar.

### 5.2 Flow

Flow rates are measured in cubic metres per hour (m<sup>3</sup>/h) at normal conditions<sup>3)</sup> taking into account the relevant conversion coefficient for the gas used (see table 2).

Table 2 — Conversion coefficient, *U*

Test gas	Conversion coefficient								
	air	oxygen	nitrogen	argon	hydrogen	helium	acetylene	LPG, e.g. propane	CO <sub>2</sub>
air	1	0,950	1,02	0,851	3,81	2,695	1,05	0,800	0,808
nitrogen	0,983	0,930	1	0,837	3,75	2,65	1,03	0,784	0,792

Conversion coefficient, *U*, is based on the formula:

$$U = \sqrt{\frac{\gamma_0}{\gamma_1}}$$

where

$\gamma_0$  is the specific weight of test gas;

$\gamma_1$  is the specific weight of gas used.

### 5.3 Temperature

Temperatures are measured in degrees Celsius.

## 6 Manufacturing requirements

### 6.1 Materials

Materials for pressure regulators shall conform to the requirements of ISO 9539.

### 6.2 Design, machining and assembly

#### 6.2.1 Oxygen regulators

Regulators for oxygen shall be designed, machined and manufactured such that internal ignition does not occur (see 11.5.3). All components and accessories shall be thoroughly cleaned and degreased before assembly.

2) Pressure exceeding atmospheric pressure.

3) Normal conditions are given in ISO 554.

## 6.2.2 Acetylene regulators

Regulators for acetylene shall be designed and manufactured so that the outlet pressure shall not exceed 1,5 bar

## 6.2.3 Filter

A dust filter, having an effective cross-section compatible with the discharge, shall be mounted within the pressure regulator upstream of the pressure regulator valve. The filter shall not be removable without the use of a tool. The filter shall retain particles greater than or equal to 0,1 mm

## 6.2.4 Outlet valve

Pressure regulators can be fitted with an outlet valve. When fitted, the spindle shall be captive.

## 6.2.5 Pressure adjusting device

This device shall be designed in such a way that it is not possible for the pressure regulator valve to be held in the open position, for example, as a consequence of the spring being compressed fully (to its solid length)

If the dimensions of the pressure adjusting screw are such as to prevent the spring becoming fully compressed, then the pressure adjusting screw shall be not removable

Using the adjusting device, it shall not be possible to set a pressure at which the relief valve vents

## 6.2.6 Relief valve

### 6.2.6.1 General

The fitting of a relief valve is obligatory for all compressed gases and carbon dioxide and optional for LPG, MPS and acetylene

The minimum discharge  $Q_{min}$  of the relief valve, if fitted, shall be equal to or greater than the standard discharge  $Q$  (see tables 3 and 4) for a pressure  $p_{rel}$  defined by the expression  $p_{rel} = 2p_1$ , except in the case of acetylene regulators, where  $p_{rel}$  shall be equal to 3 bar for all classes

With decreasing pressure the relief valve shall close at a pressure greater than  $p_1$ . The relief valve shall be non-adjustable by the user

### 6.2.6.2 Relief valve for compressed gases and carbon dioxide

The relief valve shall remain gas tight to a pressure above the maximum outlet pressure achieved when the flow is shut off for the initial pressure  $p_1$ . The relief valve shall be fitted in such a way that the gas discharges safely

### 6.2.6.3 Relief valve for acetylene

The relief valve, if fitted, shall remain gas tight to a pressure above 1,5 bar. It shall be fitted in such a way that the gas is not discharged towards to the operator.

### 6.2.6.4 Relief valve for LPG and MPS

The relief valve, if fitted, shall conform to 6.2.6.2

### **6.2.7 Pressure gauges**

When fitted externally, pressure gauges shall conform to ISO 5171. If pressure gauges are integral with the regulator, the relevant operational and safety requirements stipulated in ISO 5171 shall apply.

### **6.2.8 Gas tightness**

Pressure regulators shall be gas tight to the atmosphere and shall conform to the requirements of ISO 9090.

Pressure regulators shall be internally gas tight, i.e. between the high pressure and low pressure parts for all normal pressures for relevant gases. The maximal internal leakage shall not exceed 0,2 mbar l/min (12 cm<sup>3</sup>/h).

### **6.2.9 Mechanical resistance**

#### **6.2.9.1 Fitness for service**

Pressure regulators shall be designed and constructed in such a way that the application of pressures given in table 6 in the high pressure and low pressure chambers does not lead to permanent deformation.

#### **6.2.9.2 Safety**

Pressure regulators shall be designed and constructed so that if the low pressure chamber of the regulator, or intermediate chamber in the case of two-stage regulators, is in direct communication with a full cylinder of gas, for instance if the regulator valve is held in the open position and the outlet connection is closed (by an attached stop valve or a blind plug) the high-pressure gas shall either be safely retained or vented (see 11.5.1.2).

## **7 Types of connections**

### **7.1 Inlet connections**

Pressure regulators shall be made in such a way that the inlet connection is compatible with the cylinder valve outlet designed for the gas contained (see ISO/TR 7470). The inlet pressure  $p_1$  specified by the manufacturer, shall be not less than the maximum charging pressure (at 15 °C) permitted for the cylinder connection.

### **7.2 Outlet connections**

Threaded outlet connections shall conform to ISO 3253 and comply with the following conditions:

- the outlet connection orientation should preferably point downwards and away from the cylinder;
- curved hose tails shall not be used

## **8 Physical characteristics**

The symbols used are given in table 3.

Table 3 — Symbols used

Symbol	Explanation
$p_1$	rated (maximum) inlet pressure
$p_2$	rated (maximum) outlet pressure
$p_{2c}$	acetylene outlet pressure used for calculation of $R$ (see 11 4 4)
$p_2$	acetylene outlet pressure used for calculation of $i$ (see 11 4 5)
$p_3$	upstream pressure for type testing $p_3 = 2p_2 + 1$ bar (0.1 MPa)
$p_4$	stabilized outlet pressure (stabilization after flow ceases)
$p_5$	the highest or lowest outlet pressure during a test of determination of irregularity coefficient according to 11 4 5
$Q_1$	standard discharge
$Q_{max}$	maximum discharge
$Q_{qv}$	discharge of the relief valve
$R$	coefficient of pressure increase upon closure
$i$	irregularity coefficient

## 8.1 Pressures

### 8.1.1 Rated (maximum) inlet pressure, $p_1$

Rated (maximum) inlet pressure for which the pressure regulator is designed

### 8.1.2 Rated (maximum) outlet pressure, $p_2$

Rated (maximum) downstream pressure for the standard discharge specified in the table of equipment classes (see table 4).

NOTE — This maximum pressure is defined for testing, and is above the normal operating pressure of the pressure regulator

In the case of acetylene regulators class 2, the standard discharge will be measured at  $p_{3c}$

### 8.1.3 Stabilized outlet pressure, $p_4$ , for acetylene regulators class 2

For acetylene regulators class 2 the stabilized outlet pressure  $p_4$  shall not exceed 1.5 bar for all inlet pressures

## 8.2 Flow rates

### 8.2.1 Maximum discharge, $Q_{max}$

The maximum discharge of the gas concerned, expressed in (m<sup>3</sup>/h), which the pressure regulator can provide for an upstream pressure  $p_3$  is defined by the expression:

$$p_3 = 2p_2 + 1 \text{ bar.}$$

This discharge  $Q_{max}$  shall be not less than  $Q_1$  (see 11 4 1)

8.2.2 Standard discharge,  $Q_1$

The standard discharge is given in table 4.

8.3 Equipment classes

Performance is measured at a standard discharge  $Q_1$  related to  $p_2$ , shown in table 4.

A pressure regulator is considered to belong to one of the classes specified in table 4 if its maximum discharge,  $Q_{max}$ , is not less than the standard discharge  $Q_1$  of the class concerned.

The values of  $p_2$  and  $Q_1$  given in table 4 are preferred values, but other values are allowed.

Table 4 — Equipment classes

Gas	Class	Rated (max.) inlet pressure $p_1$ bar (10 <sup>-1</sup> MPa)	Rated (max.) outlet pressure $p_2$ bar (10 <sup>-1</sup> MPa)	Standard discharge $Q_1$ m <sup>3</sup> /h
oxygen and other compressed gases up to 300 bar (30 MPa)	0	0 to 300 <sup>1)</sup>	2	1,5
	1		4	5
	2		6	15
	3		10	30
	4		12,5	40
dissolved acetylene	1	25	0,8	1
	2		< 1,5	5 <sup>2)</sup>
MPS	0	25 <sup>3)</sup>	1,5	1
	1		4	5
LPG	0	25 <sup>4)</sup>	1,5	1 <sup>5)</sup>
	1		4	5 <sup>5)</sup>
CO <sub>2</sub>	0	200 <sup>6)</sup>	2	2 <sup>5)</sup>
	1		4	2 <sup>5)</sup>

- 1) Pressure relating to maximum cylinder charging pressure at 15 °C
- 2) General recommendations: flow rates greater than 1 m<sup>3</sup>/h should be avoided.
- 3) Vapour pressure for MPS at 65 °C. This value may change depending on components of the gas mixture.
- 4) Vapour pressure for propane at 70 °C
- 5) Depending upon ambient conditions, the use of a heater may be necessary to achieve standard discharge with LPG and CO<sub>2</sub> gases
- 6) Pressure for CO<sub>2</sub> at 70 °C at the filling ratio of 0,667

8.4 Operating characteristics

8.4.1 Coefficient of pressure increase upon closure,  $R$

This coefficient is defined by:

$$R = \frac{p_4 - p_2}{p_2}$$

For acetylene regulators class 2,  $p_2 = p_{2n}$ . (see table 3).

where  $p_4$  is the stabilized outlet pressure (stabilization pressure) noted 1 min after discharge ceases where the acetylene regulators class 2 have been set to the initial conditions  $Q_1, p_{2n}$  for inlet  $p_1$

For standard discharge  $Q_1$ , the coefficient  $R$  of pressure increase upon closure shall be less than 0.3

#### 8.4.2 Irregularity coefficient, $i$

This coefficient is defined by:

$$i = \frac{p_5 - p_2}{p_2}$$

For acetylene regulators class 2,  $p_2 = p_{2,p}$  (see table 3)

where  $p_5$  is the highest or lowest value of the outlet pressure (see figure 2) during a test in which the inlet pressure varies from  $p_1$  to  $p_3$  for a flow equal to the standard discharge  $Q_1$  in accordance with table 4

The limits shall be:  $-0,3 < i < +0,3$ .

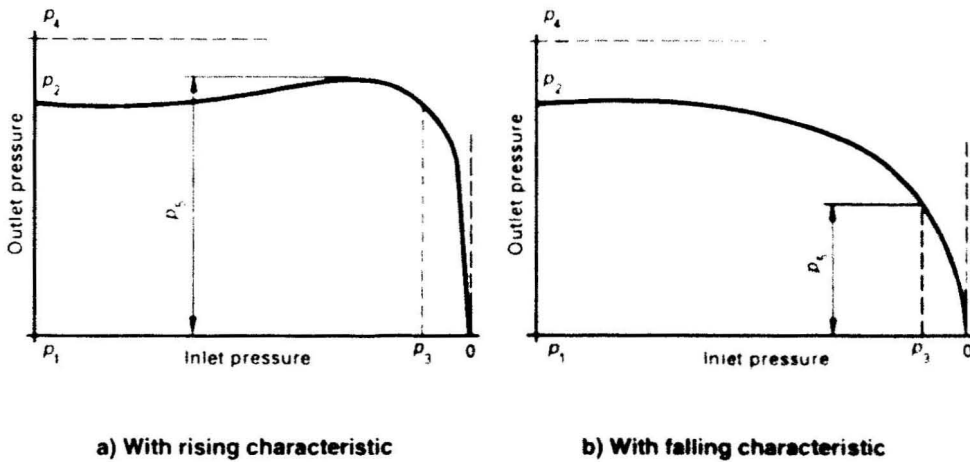


Figure 2 — Typical dynamic expansion curves

#### 8.4.3 Operating temperature range

The pressure regulators shall be capable of operating normally in the temperature range  $-20\text{ }^{\circ}\text{C}$  to  $+60\text{ }^{\circ}\text{C}$

## 9 Marking

The following information shall be clearly and permanently marked in accordance with 11.6 on the pressure regulator body or cover or on a label permanently fixed to the pressure regulator

- the number of this International Standard;
- the name or trade mark of the manufacturer and/or distributor;
- pressure regulator class or  $p_1, Q_1$  in accordance with 8.3.

- rated inlet pressure,  $p_1$ , nominated by the manufacturer (only for oxygen and other compressed gases);
- gas intended for use (when the full name of the gas cannot be imprinted the symbols shown in table 5 shall be used).

**Table 5 — Code letters for gases to be used for marking of pressure regulators**

Type of gas	Code letter
acetylene	A
oxygen	O
hydrogen	H
compressed air	D
LPG	P
MPS	Y
natural gas	M
CO <sub>2</sub> , nitrogen, inert gas	N

## 10 Instructions for use

The manufacturer, supplier or distributor shall supply instructions for use with each pressure regulator, covering at least:

- the field of application of the pressure regulator;
- a description of the pressure regulator and the meaning of the marking;
- the safe and correct installation of the pressure regulator;
- the commissioning tests that are necessary to guarantee safe and correct installation prior to service;
- the use and maintenance of the pressure regulator (intended for the operator), including hazards and safety precautions in the case of oxygen

## 11 Type test procedure

### 11.1 General

Checking conformity to this International Standard, of a regulator of a given type consists of:

- tests;
- checking of documents

Conformity to the requirements of this International Standard can be confirmed by an independent body.

The oxygen ignition test (see 11.5.3) shall be carried out after the functional tests (see 11.4) and before the fitness test (see 11.5.1.1).

**NOTE** — These tests are applicable only to regulators submitted for conformity to this International Standard, i. e. type tests, and are not intended as the programme for production testing of all regulators.

## 11.2 Test samples and necessary documents

For the tests the following samples and documents shall be available:

- 3 samples of the pressure regulator (five in the case of oxygen).
- 1 set of general arrangement drawings with material lists;
- 2 sets of detailed drawings;
- if necessary a declaration from the manufacturer giving the material specifications and fitness for purpose.

The tests shall be carried out with pressure regulators which are in accordance with the drawings.

## 11.3 Test conditions

### 11.3.1 General characteristics of the test installation

All the pipelines of the testing installation together with the valve which controls the flow shall have a passage greater than that of the regulator to be tested.

### 11.3.2 Type of gas

Tests shall be carried out with air or nitrogen free from oil and grease in accordance with ISO 554.

Only the ignition test according to 11.5.3 shall be carried out with oxygen.

In all cases, tests shall be carried out with a gas of maximum moisture content of 0.005 % corresponding to a dew point of  $-48\text{ }^{\circ}\text{C}$ .

### 11.3.3 Units of measurement and rating test

Flow measurement data shall be expressed in accordance with the specifications contained in ISO 554.

The tolerance of the measuring apparatus shall not exceed  $\pm 3\%$  of the measuring range.

### 11.3.4 Pressure measurement

The test bench shall be constructed in such a way that upstream and downstream pressures can be regulated. The equipment may be operated by remote control.

The gas supply for the rated (maximum) inlet pressure  $p_1$  and for pressure  $p_2$  shall have sufficient capacity for the duration of the test.


Gauges of class 1 or better shall be used for the pressure measurement. In such cases, the pressure gauges on the regulators can be included in the testing.

## 11.4 Functional tests

### 11.4.1 General

An example of the test apparatus used for the measurement of the maximum discharge,  $Q_{max}$ , is shown in figure 3. The pressure regulator may be supplied via a buffer cylinder. The upstream pressure  $p_1$  (see 8.2.1) is held constant by means of an auxiliary regulator or any equivalent device.



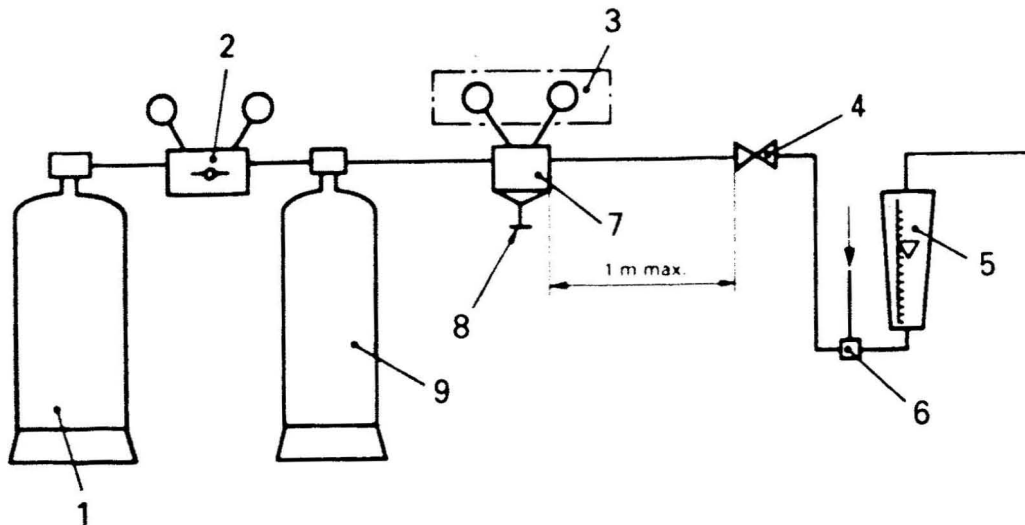

**Key**

- |                        |  |
|------------------------|--|
| 1 Gas supply           | 6 Thermometer for measurement of the gas temperature |
| 2 Auxiliary regulator  | 7 Regulator (sample)                                 |
| 3 Calibrated gauges    | 8 Adjusting screw                                    |
| 4 Valve for regulation | 9 Buffer cylinder                                    |
| 5 Flowmeter            |  |

**Figure 3 — Example for the measurement of the maximum discharge,  $Q_{max}$ .**

**11.4.2 Maximum discharge,  $Q_{max}$ .**

The maximum discharge,  $Q_{max}$ , shall be measured as follows

**11.4.2.1 Maximum discharge,  $Q_{max}$ , excluding acetylene regulators class 2**

The adjusting screw of the regulator sample under test shall be fully screwed in, and the valve for regulation shall be fully opened so that

- the downstream pressure gauge indicates the rated (maximum) outlet pressure  $p_r$ ,
- flowmeter indicates the maximum discharge,  $Q_{max}$ , taking into account the corrections in 11.3.3 and table 2 and the temperature measured by the thermometer

**11.4.2.2 Maximum discharge,  $Q_{max}$ , for acetylene regulators class 2**

The adjusting screw of the regulator sample under test shall be fully screwed in, and the valve for regulation shall be fully opened. The flowmeter indicates the maximum discharge,  $Q_{max}$ , taking into account the corrections in 11.3.3 and table 2 and the temperature measured by the thermometer

NOTE —  $Q_{max}$  defined in 8.2.1 is a conventional value. It may be lower than the real flow, which the regulator may permit under different conditions.

**11.4.3 Standard discharge,  $Q_s$ .**

The standard discharge,  $Q_s$ , shall be obtained using the following settings.

#### 11.4.3.1 Standard discharge, $Q_s$ , excluding acetylene regulators class 2

The adjusting screw of the regulator sample under test and the valve for regulation shall be set to achieve  $p_2$ ,  $Q_s$  at  $p_3$  inlet

#### 11.4.3.2 Standard discharge, $Q_s$ , for acetylene regulators class 2

The adjusting screw of the regulator sample under test shall be fully screwed in, and the valve for regulation shall be opened to achieve  $Q_s$  at  $p_3$  and the corresponding outlet pressure measured. This pressure shall be referred to as  $p_{2s}$

#### 11.4.4 Coefficient of pressure increase upon closure, $R$


With the regulator set to standard discharge conditions (see 11.4.3) proceed as follows

- stop the flow by using the valve for regulation;
- after 1 min record the stabilization pressure  $p_2$ ;
- determine the value of  $R$  (see 8.4.1).

#### 11.4.5 Irregularity coefficient, $i$

For the determination of the irregularity coefficient,  $i$ , (see 8.4.2) a dynamic expansion curve is plotted. This curve indicates the downstream pressure as a function of the upstream pressure. During this test the upstream pressure varies from the rated (maximum) inlet pressure  $p_1$  to pressure  $p_2$ .

An example of the test apparatus is shown in figure 4

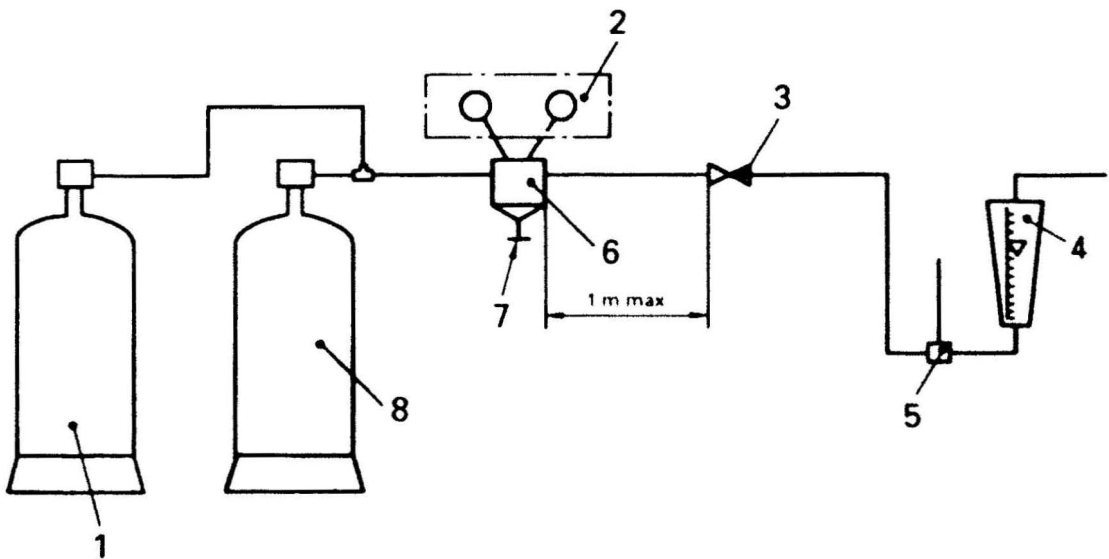

**Key**

- |  |  |
|--|--|
| 1 Auxiliary gas cylinder                   | 5 Thermometer for measurement of the gas temperature |
| 2 Calibrated gauges or recording equipment | 6 Regulator (sample)                                 |
| 3 Valve for regulation                     | 7 Adjusting screw                                    |
| 4 Flowmeter                                | 8 Primary gas cylinder                               |

Figure 4 — Example for the measurement of the dynamic expansion curves

The pressure regulator is equipped with two calibrated pressure gauges, preferably recording gauges<sup>4)</sup>. The regulator is supplied by two gas cylinders, where at any given time only one cylinder is in operation. Both cylinders are filled with test gas under the rated (maximum) inlet pressure  $p_1$ . The pressure regulator discharge is controlled by a flowmeter.

#### 11.4.5.1 Pre-test settings excluding acetylene regulators class 2

The adjusting screw of the regulator sample under test and the valve for regulation shall be set to achieve  $p_2$ ,  $Q_1$  at  $p_1$  inlet.

#### 11.4.5.2 Pre-test settings for acetylene regulators class 2

The adjusting screw of the regulator sample under test shall be fully screwed in and inlet pressure  $p_1$  shall be adjusted by means of the regulator valve to achieve  $Q_1$ , the resulting outlet pressure shall be measured and referred to as  $p_2$ .

#### 11.4.5.3 Tests

Without changing the preceding setting, the cylinder valve of the auxiliary cylinder shall be closed and that of the primary cylinder shall be opened. At this time, the values of the upstream and downstream pressures are recorded. The capacity of the primary cylinder shall be sufficient for a test period of at least 15 min.

However, if the pretest settings can be achieved in less than 30 s and the auxiliary cylinder has sufficient capacity, the test can be carried out without switching to the primary cylinder.

#### 11.4.5.4 Results

During this test there shall be no evidence of oscillation or sticking of the pressure regulator and there shall be a smooth regulator dynamic expansion curve, either rising to a maximum (see figure 2a) or falling (see figure 2b).

The pressure  $p_i$  for the irregularity coefficient  $i$ , is the highest or lowest value of the outlet pressure during the test in which the inlet pressure varies from  $p_1$  to  $p_1$ .

Determine the value of  $i$  (see 8.4.2)

### 11.5 Mechanical tests

**WARNING** — Precautions shall be taken to protect test personnel.

#### 11.5.1 Internal pressure tests

##### 11.5.1.1 Fitness test

For this test (see 6.2.9.1) the relief valve, diaphragm and pressure gauges shall be replaced by blind plugs. The low and high pressure chambers shall be hydraulically pressurized for 5 min. After the test, check that there is no permanent deformation (for example measured by comparison)

The test pressures are given in table 6

Table 6 — Test pressures

Gas	High pressure chambers	Low pressure chambers
oxygen and other compressed gases, $p_1$ up to 20 bar, classes 0, 1, 2, 3, 4 and 5	$1.5 \times p_1$	60 bar (6 MPa)
acetylene classes 1 and 2	300 bar (30 MPa)	30 bar (3 MPa)
LPG and MPS classes 0 and 1		
CO <sub>2</sub> classes 0 and 1		60 bar (6 MPa)

4) Or any other recording device which produces the dynamic expansion curve directly

### 11.5.1.2 Safety test

For this test (see 6.2.9.2), the pressure regulator valve shall be held permanently open or removed. The pressure gauges shall be replaced by blind plugs and the outlet blanked off.

A pneumatic pressure of  $p_1$  shall be applied to the regulator inlet, through a valve which is manually opened quickly.

If no rupture occurs, the test is satisfactory.

If rupture occurs, no pieces shall be ejected. Venting of gas through pressure relief devices, if fitted, is allowed.

### 11.5.2 Leakage tests

Gas tightness to the atmosphere shall be tested in accordance with ISO 9090.

Gas tightness of the regulator valve assembly:


- The gas tightness of the regulator valve seat is tested at the maximum inlet pressure  $p_1$  for 5 min. The regulator valve shall be closed (pressure adjusting screw completely unscrewed) and the outlet open. An escape of gas of 0,2 mbar l/min (12 cm<sup>3</sup>/h) is allowed.
- The gas tightness of the regulator valve is also tested with the outlet closed and the pressure in the low pressure chamber adjusted to the value  $p_2$  with the pressure adjusting screw. The value of  $p_2$  shall be constant during the test period of 5 min.

Both tests shall be repeated with the critical test pressure  $p_c$ .

### 11.5.3 Ignition test (oxygen pressure regulators)

Three samples of the oxygen pressure regulator shall be exposed, through their inlets, to pressure shocks from industrial oxygen (minimum 99,5 % purity; hydrocarbons  $\leq$  0,001 %). The test system (see figure 5) shall be provided with equipment for preheating the oxygen, an oxygen vessel and a quick opening valve. Figure 5 gives an example of test bench

Dimensions in millimetres

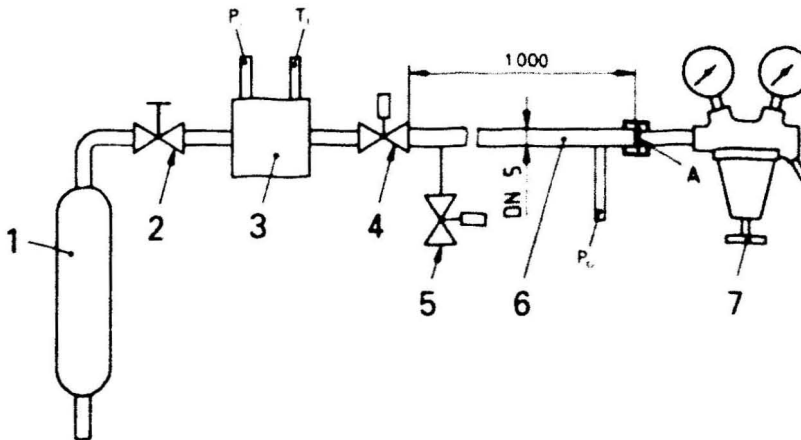

#### Key

- |   |   |
|---|---|
| 1 Oxygen supply   | 6 Connection tube                                       |
| 2 Inlet valve   | 7 Test sample pressure regulator                        |
| 3 Oxygen vessel with preheating device<br>(e.g. water bath, electric heating) | P <sub>1</sub> Pressure transducer on the oxygen vessel |
| 4 Quick opening valve   | P <sub>2</sub> Pressure transducer on the outlet valve  |
| 5 Outlet valve  | T <sub>1</sub> Thermoelement                            |
|   | A Measuring point                                       |

Figure 5 — Test bench for ignition test

The time required to increase the pressure from atmospheric to the test pressure shall be  $(20_{-5}^0)$  ms, measured at point A prior to the test (see figure 5).

The pressure shall also be measured at a distance of 30 mm to 40 mm from the sealing face of the sample ( $P_o$ , see figure 5). At least every second pressure shock shall be recorded. The connection tube between the quick opening valve and the regulator under test shall be 1 000 mm in length and 5 mm in internal diameter. Before the test is started, the samples shall be at room temperature. The test pressure shall in all cases, be  $1,2 \times p_1$  at a temperature of  $(60 \pm 3) ^\circ\text{C}$ .

Each test series shall consist of 20 pressure shocks at intervals of 30 s (see figure 6).

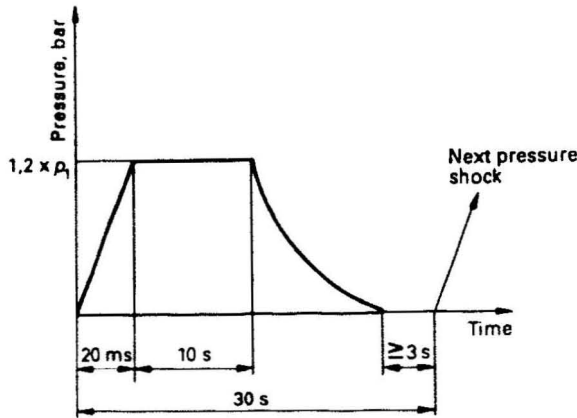


Figure 6 — Test interval

Each pressure shock is applied for 10 s. After each pressure shock, the pressure regulator is brought back to atmospheric pressure. This shall not be done by adjusting the regulator, but by operating an upstream outlet valve. Between each pressure shock, atmospheric pressure shall be held for at least 3 s.

During a test series, the inlet pressure (test pressure) shall not decrease by more than 3 %.

The tests shall be carried out under the following conditions:

- a) with the regulator valve in the fully opened position and outlet closed;
- b) with the regulator valve in the fully closed position.

The regulator shall not burn out during the test. After the tests have been completed, the three test samples shall be dismantled and all internal parts and surfaces inspected. Internal damage and evidence of burning are not acceptable.

#### 11.5.4 Relief valve

For the test, the regulator valve shall be fully opened or removed. The outlet of the regulator shall be blanked off. An increasing pressure is applied through the inlet up to pressure given in 6.2.6. At this pressure, the relief valve shall be leak-tight. The pressure shall then be increased to the opening pressure of the relief valve which shall then be noted. The pressure shall be increased to the pressure  $p_{rv} = 2p_2$ . At this pressure, the discharge  $Q_{rv}$  of the relief valve shall be measured (see 6.2.6).

#### 11.6 Test for durability of markings

Markings shall be rubbed by hand, without undue pressure, first for 15 s with a cloth soaked with distilled water, then for 15 s with a cloth soaked with petroleum spirit. Labels, if used as markings, shall be adhesive over the whole attachment surface.

After the test, the marking shall remain legible.

**NATIONAL ANNEX A**  
( *National Foreword* )

**A-1 BIS CERTIFICATION MARKING**

The products may also be marked with the Standard Mark.

**A-1.1** The use of the Standard Mark is governed by the provisions of the *Bureau of Indian Standards Act, 1986* and the Rules and Regulations made thereunder. The details of conditions under which the licence for the use of the Standard Mark may be granted to manufacturers or producers may be obtained from the Bureau of Indian Standards.

## Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act, 1986* to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

### Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in the course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

### Review of Indian Standards

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard alongwith amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the latest issue of 'BIS Catalogue' and 'Standards: Monthly Additions'.

This Indian Standard has been developed from Doc: No. MTD 11 (4740).

### Amendments Issued Since Publication

Amend No.	Date of Issue	Text Affected

## BUREAU OF INDIAN STANDARDS

### Headquarters

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110002

Telephones 2323 0131, 2323 3375, 2323 9402

Website: [www.bis.org.in](http://www.bis.org.in)

### Regional Offices

		Telephones
Central	Manak Bhavan, 9 Bahadur Shah Zafar Marg NEW DELHI 110002	2323 7617 2323 3841
Eastern	1/14 C.I.T. Scheme VII M, V.I.P. Road, Kankurgachi KOLKATA 700054	2337 8499, 2337 8561 2337 8626, 2337 9120
Northern	SCO 335-336, Sector 34-A, CHANDIGARH 160022	260 3843 260 9285
Southern	C.I.T. Campus, IV Cross Road, CHENNAI 600113	2254 1216, 2254 1442 2254 2519, 2254 2315
Western	Manakalaya, E9 MIDC, Marol, Andheri (East) MUMBAI 400093	2832 9295, 2832 7858 2832 7891, 2832 7892

### Branches

AHMEDABAD BANGALORE BHOPAL BHUBANESHWAR COIMBATORE FARIDABAD  
GHAZIABAD GUWAHATI HYDERABAD JAIPUR KANPUR LUCKNOW NAGPUR  
PARWANOO PATNA PUNE RAJKOT THIRUVANANTHAPURAM VISAKHAPATNAM.